

EC DECLARATION OF CONFORMITY

Name and address of the manufacturer: / **F. Y. Z. C. CO.,LTD**
Chengxiyuan, economic development zone, Youxi County, Fujian Province

EC Authorized Representative:/ **Caretechion GmbH**
Niederrheinstr 71,40474 Duesseldorf, Germany

We declare under our sole responsibility that:

Name of the medical device: / **Disposable surgical mask**

Type: / **Type IIR**

Product code:/ **UMDNS code 12458 (Masks, Surgical)**

Intended purpose: / **The Disposable surgical mask is intended to be worn to protect against the spread or transmission of infectious germs during surgical interventions in operating theatres and other medical facilities. The main aim is to protect the patient against infectious germs. In addition, in certain situations the wearer should be protected against splashes of potentially contaminated liquids and viable particles.**

Basic UDI-DI:/ **NA**

Trade name:/ **None**

of class: / **Rule1, Class I**
according to annex VIII of Regulation (EU) 2017/745 /

CS reference: / **NONE**

Applicable standards: / **EN 14683:2019**
EN ISO 10993-5:2009
EN ISO 10993:10:2013

Conformity assessment: / **Declare the conformity of the abovementioned products by issuing this EU Declaration of Conformity after drawing up the technical documentation set out in Annexes II and III of Regulation (EU) 2017/745 /**
according to Article 52(7) of Regulation (EU) 2017/745 /

Meets the provisions of the Regulation EU 2017/745(MDR) which apply to it. The declaration is valid in connection with the "final inspection report" of the device. /

CE

Fujian P.R. May 21th. 2020

Ort. Datum / Place, date /
Lieu, date / Luogo, data

Zheng Xu, Manager

Name und Funktion / Name and function /
Nom et fonction / Nome e funzione





SUBJECT Physical & Microbiological Test

TEST LOCATION TÜV SÜD China
TÜV SÜD Products Testing (Shanghai) Co., Ltd.
B-3/4, No.1999 Du Hui Road, Minhang District
Shanghai 201108, P.R. China

CLIENT NAME F.Y.Z.C. CO.,LTD

CLIENT ADDRESS Chengxiyuan,economic development zone,Youxi County,Fujian Province

TEST PERIOD 17-Apr-2020~02-May-2020

Prepared By

Bella Xu

(Bella Xu)
Report Drafter

Authorized By



(Leo Liu)
Authorized Signatory

Note: (1) General Terms & Conditions as mentioned overleaf. (2) The results relate only to the items tested.(3) The test report shall not be reproduced except in full without the written approval of the laboratory.(4) Without the agreement of the laboratory, the client is not authorized to use the test results for unapproved propaganda.

Chemical/Microbiology Laboratory:
TÜV SÜD Products Testing (Shanghai) Co.,
Ltd.
B-3/4, No.1999 Du Hui Road, Minhang District
Shanghai
201108
P.R. China

Phone : +86 (21) 6037 6375
Fax : +86 (21) 6037 6345
Email: food.chem@tuv-sud.cn
Webpage: www.tuv-sud.cn

Regional Head Office:
TÜV SÜD Certification and Testing
(China) Co., Ltd.
No.151 Heng Tong Road Shanghai
200 070 P.R.China

TUV®

TEST REPORT

Sample Description : Disposable surgical mask
Sample Quantity : 60 pieces
Lot Number/Batch Code : 20200325
Specification : /
Size : 175mm x 95mm
Brand Name : /

Remark: The above information was provided by applicant.

Summary of Test Results

No.	Test Item	Test Method	Test Standard Type II R	Judgement
1	Bacterial Filtration Efficiency Test (BFE), %	EN 14683:2019+AC:2019(E) Annex B	≥ 98	Pass
2	Differential Pressure Test (Pa/cm ²)	EN 14683:2019+AC:2019(E) Annex C	< 60	Pass
3	Synthetic Blood Penetration Test (kPa)	ISO 22609:2004	≥ 16.0	Pass
4	Microbial Cleanliness Test (CFU/g)	EN 14683:2019+AC:2019(E) Annex D	≤ 30	Pass

Note: Pass = Meet customer requirements;

Fail = Fail customer requirements;

= No comment;

N.D. = Not detected.

Photo of Samples



Results

No.	Test Item	Test Result
1	Bacterial Filtration Efficiency (BFE) Test	Specimen 1#: 99.9% Specimen 2#: 99.9% Specimen 3#: 99.9% Specimen 4#: 99.9% Specimen 5#: 99.9%
2	Differential Pressure Test	27.0 Pa/cm ²
3	Synthetic Blood Penetration Test	Specimen 1#~32#: None seen
4	Microbial Cleanliness Test	Specimen 1#: <1 CFU/g Specimen 2#: 2 CFU/g Specimen 3#: 3 CFU/g Specimen 4#: <1 CFU/g Specimen 5#: 1 CFU/g

Bacterial Filtration Efficiency (BFE) Test

1. Purpose

For evaluating the bacterial filtration efficiency (BFE) of mask.

2. Sample description was given by client

Sample description : Disposable surgical mask
Specification : /
Lot Number : 20200325
Sample Receiving Date : 2020-04-17

3. Test Method

EN 14683:2019+AC:2019(E) Annex B

4. Apparatus and materials

- 4.1 *Staphylococcus aureus* ATCC 6538.
- 4.2 Peptone water.
- 4.3 Tryptic Soy Broth(TSB).
- 4.4 Tryptic Soy Agar(TSA).
- 4.5 Bacterial filtration efficiency test apparatus.
- 4.6 Six-stage viable particle Anderson sampler.
- 4.7 Flow meters.

5. Test specimen

- 5.1 As requested by client, take a total of 5 test specimens.
- 5.2 Prior to testing, condition all test specimens for a minimum of 4 h at (21±5)°C and (85±5)% relative humidity.

6. Procedure

- 6.1 Preparation of the bacterial challenge: Dilute the culture in peptone water to achieve a concentration of approximately 5×10^5 CFU/mL.
- 6.2 Adjust the flow rate through the Anderson sampler to 28.3 L/min.
- 6.3 Deliver the challenge to the nebulizer using a syringe pump. Purge tubing and nebulizer of air bubbles.
- 6.4 Perform a positive control run without a test specimen to determine the number of viable aerosol particles being generated. The mean particle size (MPS) of the aerosol will also be calculated from the results of these positive control plates.
 - 6.4.1 Initiate the aerosol challenge by turning on the air pressure and pump connected to the nebulizer. Immediately begin sampling the aerosol using the Anderson sampler.
 - 6.4.2 Time the challenge suspension to be delivered to the nebulizer for 1 min.
 - 6.4.3 Time the air pressure and Anderson sampler to run for 2 min.
 - 6.4.4 At the conclusion of the positive control run, remove plates from the Anderson sampler.
- 6.5 Place new agar plates into Anderson sampler and clamp the test specimen into the top of the Anderson sampler, with the inside of the specimen facing towards the bacterial challenge (test area: 77cm^2).
- 6.6 Repeat the challenge procedure for each test specimen.
- 6.7 Repeat a positive control after completion of the sample set.
- 6.8 Perform a negative control run by collecting a 2 min sample of air from the aerosol chamber. No bacterial challenge should be pumped into the nebulizer during the collection of the negative control.
- 6.9 Incubate agar plates at $(37 \pm 2)^\circ\text{C}$ for (20 to 52) h.
- 6.10 Count each of the six-stage plates of the Anderson sampler.

7. Calculation

Total the count from each of the six plates for the test specimens and positive controls, as specified by the manufacture of Anderson sampler. The filtration efficiency percentages are calculated as follows:

$$\text{BFE} = (C - T) / C \times 100$$

T is the total plate count for the test specimen.

C is the mean of the total plate counts for the two positive controls.



8. Test results*

<i>P</i> Value Stage Number	Positive Control (A)	Positive Control (B)	Negative Control	Specimen 1#	Specimen 2#	Specimen 3#	Specimen 4#	Specimen 5#
1	19	45	0	0	0	0	0	0
2	41	78	0	0	0	0	0	0
3	101	131	0	0	0	0	0	0
4	206	256	0	0	0	0	0	0
5	1179	1371	0	0	0	0	0	0
6	739	513	0	0	0	0	0	0
Total (<i>T</i>), CFU	2285	2394	<1	<1	<1	<1	<1	<1
Average (<i>C</i>), CFU	$2.3 \times 10^3 = (P_A + P_B) / 2$							
BFE, %				99.9	99.9	99.9	99.9	99.9
Requirements	≥ 98							
Remarks	<i>P</i> is the value of corresponding corrected particle counts as specified by the manufacturer of the cascade impactor. <i>T</i> is the total of <i>P</i> value for the test specimen. <i>C</i> is the mean of the total of <i>P</i> value of the two positive controls.							

Differential pressure Test

1. Purpose

The purpose of the test was to measure the differential pressure of masks.

2. Sample description was given by client

Sample description : Disposable surgical mask
Specification : /
Lot Number : 20200325
Sample Receiving Date : 2020-04-17

3. Test Method

EN 14683:2019+AC:2019(E) Annex C

4. Apparatus and materials

Differential pressure testing instrument

5. Test specimen

- 5.1 Test specimen are complete masks or shall be cut from masks. Each specimen shall be able to provide 5 different circular test areas of 2.5 cm in diameter.
5.2 Prior to testing, condition all test specimens for a minimum of 4 h at (21±5) °C and (85±5)% relative humidity.

6. Procedure

- 6.1 Without a specimen in place, the holder is closed and the differential manometer is zeroed. The pump is started and the flow of air adjusted to 8 L/min.
6.2 The pretreated specimen is placed across the orifice (total area 4.9cm², test area diameter 25mm) and clamped into place so as to minimize air leaks.
6.3 Due to the presence of an alignment system the tested area of the specimen should be perfectly in line and across the flow of air.
6.4 The differential pressure is read directly.
6.5 The procedure described in steps 6.1-6.4 is carried out on 5 different areas of the mask and readings averaged.

Results:

Specimen	Test Results* (Pa/cm ²)	Average (Pa/cm ²)	Requirements	Judgement
1#	27.7	27.0	< 60	Pass
2#	25.6			
3#	27.4			
4#	28.0			
5#	26.5			

TUV
SUD
告
1
*

Synthetic Blood Penetration Test

1. Purpose

For evaluation of resistance of masks to penetration by a fixed volume of synthetic blood at a high velocity.

2. Sample description was given by client

Sample description : Disposable surgical mask
Specification : /
Lot Number : 20200325
Sample Receiving Date : 2020-04-17

3. Test Method

ISO 22609:2004

4. Apparatus and materials

- 4.1 Synthetic blood.
- 4.2 Tensiometer.
- 4.3 Synthetic blood penetration test apparatus;
- 4.4 Targeting plate.
- 4.5 Air pressure source.
- 4.6 Ruler.
- 4.7 Balance.
- 4.8 Controlled temperature and humidity chamber.

5. Test specimen

- 5.1 As requested by client, take a total of 32 test specimens.
- 5.2 Prior to testing, condition all test specimens for a minimum of 4h at $(21\pm 5)^{\circ}\text{C}$ and $(85\pm 5)\%$ relative humidity.

6. Procedure

- 6.1 Prepare the synthetic blood (40~44 mN/m) for the test.
- 6.2 Determine the density of the synthetic blood.
- 6.3 Fill the reservoir with new synthetic blood.
- 6.4 Position the test specimen 30.5 cm (12 in.) from the exit of the canula.
- 6.5 Set the reservoir pressure to the approximate pressure.
- 6.6 Place the targeting plate approximately 1 cm away from the mask.
- 6.7 Set the valve timer to 0.5 s. Collect and weigh the amount of fluid delivered (before the targeting

- hole).
- 6.8 Set the valve timer to 1.5 s. Collect and weigh the amount of fluid delivered (before the targeting hole).
- 6.9 Calculate the difference in weight of the two spurts. For a test fluid with a density of 1.003, Table 1 gives the target difference in weight plus lower and upper limits for a velocity range within 2% of the target.

Table 1 Target weight difference

Fluid Pressure (mmHg)	Weight difference for 1s difference in spurt duration (g)		
	Min.	Target	Max.
120	3.002	3.063	3.124

- 6.10 Adjust the reservoir pressure and repeat steps 6.7 to 6.9 until the weight difference is within the target range.
- 6.11 Record the weight difference for the spurts exiting the nozzle.
- 6.12 Record the pressure in the reservoir.
- 6.13 Set the valve time to 0.5 s. Collect and weigh the amount of fluid passing through the targeting hole.
- 6.14 Set the valve time to 1.5 s. Collect and weigh the amount of fluid passing through the targeting hole.
- 6.15 The difference in weight between the 0.5 s and 1.5 s spurts through the targeting plate shall be within +2 % ~ -5 % of the difference in weight from the nozzle.
- 6.16 If the differential weight is less than 95 % of the weight difference exiting the nozzle, check the aim of the stream to make sure it is passing cleanly through the targeting hole.
- 6.17 If the differential weight is more than 102 % of the weight difference exiting the nozzle, repeat the weight measurements exiting the nozzle (steps 6.7 to 6.11).
- 6.18 For standard synthetic blood, the timer duration can be estimated using the formula:
(p is the density of the test fluid.) $t = 0.5 + (2 \times p - g \text{ at } 0.5 \text{ s}) / (g \text{ at } 1.5 \text{ s} - g \text{ at } 0.5 \text{ s})$.
- 6.19 Record the timer setting to use as the starting point for subsequent testing.
- 6.20 Mount a test specimen on the specimen holding fixture. If the mask contains pleats, spread the pleats out when mounting the mask onto the fixture to present a single layer of material as the target area.
- 6.21 Squirt the synthetic blood onto the test specimen for the calculated time. Ensure that the synthetic blood hits the target area of mask.
- 6.22 Inspect the inside surface for synthetic blood penetration within 10 s of squirting the synthetic blood against the target area.
- 6.23 Report the results (none / penetration) for each test specimen at the test pressure.



Results:

Specimen	Test Results*	Requirements	Judgement
1#	None Seen	Pass Pressure at 16.0 kPa (120mmHg)	Pass
2#	None Seen		Pass
3#	None Seen		Pass
4#	None Seen		Pass
5#	None Seen		Pass
6#	None Seen		Pass
7#	None Seen		Pass
8#	None Seen		Pass
9#	None Seen		Pass
10#	None Seen		Pass
12#	None Seen		Pass
13#	None Seen		Pass
14#	None Seen		Pass
15#	None Seen		Pass
16#	None Seen		Pass
17#	None Seen		Pass
18#	None Seen		Pass
19#	None Seen		Pass
20#	None Seen		Pass
22#	None Seen		Pass
23#	None Seen		Pass
24#	None Seen		Pass
25#	None Seen		Pass
26#	None Seen		Pass
27#	None Seen		Pass
28#	None Seen		Pass
29#	None Seen		Pass
30#	None Seen		Pass
31#	None Seen		Pass
32#	None Seen		Pass

Microbial Cleanliness Test

1. Purpose

The purpose of the test was to measure microbial cleanliness of mask.

2. Sample description was given by client

Sample description : Disposable surgical mask
Specification : /
Lot Number : 20200325
Sample Receiving Date : 2020-04-17

3. Test Method

According to EN ISO 11737-1:2018 to determine the microbial cleanliness of mask material, and refer to the procedure as described in EN 14683:2019+AC:2019(E) Annex D

4. Apparatus and materials

- 4.1 Orbital shaker.
- 4.2 0.45 um filter.
- 4.3 Tryptic Soy Agar (TSA).
- 4.4 Sabouraud Dextrose Ager (SDA) with chloramphenicol.
- 4.5 Formula of Extraction Liquid: 1g/L peptone, 5g/L NaCl and 2g/L Tween 20.
- 4.6 Extraction apparatus.

5. Test specimen

- 5.1 As requested by client, take a total of 5 mask samples.
- 5.2 Mask samples for testing are provided in the original primary packaging.
- 5.3 Condition at (18 to 26)°C and (45 to 65)% relative humidity during testing.

6. Procedure

- 6.1 Five test specimens are selected from the top, bottom and 3 randomly chosen marks.
- 6.2 The mask is aseptically removed from the packaging and placed in a sterile 500 mL bottle containing 300 mL of extraction liquid.
- 6.3 The bottle is laid down on an orbital shaker and shaken for 5 min at 250 rpm.
- 6.4 After extracting, 100mL of the extraction liquid is filtered through a 0.45 um filter and laid down on a TSA plate for the total viable aerobic microbial count. Another 100 mL aliquot of the same extraction liquid is filtered in the same way and the filter plated on SDA for fungi enumeration.
- 6.5 The plates are incubated for 3 days at 30°C and 7 days at (20 to 25)°C for TSA and SDA plates respectively.
- 6.6 Calculate the colonies of each agar plate.

7. Calculation

For each test specimen calculate the microbial cleanliness as follows by counting the total colonies of the TSA and SDA plates.



Results*:

Specimen	Colonies of the TSA Plate	Colonies of the SDA Plate	Microbial Cleanliness, (CFU/g)	Requirements	Judgement
1#	0	0	<1	EN14683:2019+AC:2019(E) Annex D EN ISO 11737-1:2018 ≤ 30 CFU/g	Pass
2#	0	2	2		
3#	0	3	3		
4#	0	0	<1		
5#	0	1	1		

Note:

- 1.*denotes this test was carried out by external laboratory assessed as competent.
- 2.This report is for internal use only such as internal scientific research ,education, quality control, product R&D.

-END OF THE TEST REPORT-





中国认可
国际互认
检测
TESTING
CNAS L3428

Test Report

Date: 2020-06-01
No. : DY20040404

TEST FACILITY

STC (Dongguan)
68 Fumin Nan Road, Dalang,
Dongguan, Guangdong,
China. (Zip code 523770)

SPONSOR

TÜV SÜD Certification and Testing (China) Co., Ltd.
Guangzhou Branch
5F, Communication Building, 163 Pingyun Rd,
Huangpu West Ave, Guangzhou 510656 P. R. China

SUPPLIER

F. Y. Z. C. CO.,LTD
Chengxiyuan,economic development zone,Youxu
County,Fujian Province

CONFIDENTIAL

STUDY TITLE

Guinea Pig Maximization Sensitization Test

TEST ARTICLE NAME

Disposable surgical mask

TEST ARTICLE IDENTIFICATION

CP-MD-2176

CSD No.: CL20200402470

STC (Dongguan) Company Limited

68 Fumin Nan Road, Dalang, Dongguan, Guangdong, China. Zip Code: 523770
Tel : (86 769) 81119888 Fax : (86 769) 81116222 Email : dgstc@stc.group Website : www.stc.group
This report shall not be reproduced unless with prior written approval from STC (Dongguan) Company Limited.
For Conditions of Issuance of this test report, please refer to the overleaf and Website.



Test Report

Date: 2020-06-02
No.: DY20040402

Summary

The test article, Disposable surgical mask, was evaluated for potential cytotoxic effects. This study was conducted following the guidelines of ISO 10993-5, Biological evaluation of medical devices - Part 5: Tests for in vitro cytotoxicity (2009). A single preparation of the test article was extracted in single strength Minimum Essential Medium at 37°C for 24 hours. The negative control, reagent control, and positive control extracts were similarly extracted. Triplicate monolayers of L-929 mouse fibroblast cells were dosed with each extract and incubated at 37°C in the presence of 5% CO₂ for 24 hours. Following incubation, the monolayers were examined microscopically for abnormal cell morphology and cellular degeneration.

The MEM test extract showed discrete intracytoplasmic granules, no cell lysis, no reduction of cell growth. The test article extract met the requirements of the test since the grade was not greater than 2(Mild).

Authorized Signatory Approval: _____

Tang

Jonathan Tang



STC (Dongguan) Company Limited

68 Fumin Nan Road, Dalang, Dongguan, Guangdong, China. Zip Code: 523770
Tel : (86 769) 81119888 Fax : (86 769) 81116222 Email : dgstc@stc.group Website : www.stc.group
This report shall not be reproduced unless with prior written approval from STC (Dongguan) Company Limited.
For Conditions of Issuance of this test report, please refer to the overleaf and Website.

15mm

105mm

80mm

72mm

15mm

200mm

105mm


200mm

105mm

50 pcs

MASCARILLA QUIRURGICA IIR DESECHABLE

DISPOSABLE SURGICAL MASK IIR



Disposable Surgical Mask IIR



C/ Sofia, 3-5 - Pol. Ind. Cabezo Beaza
30353 Cartagena (Spain)

F. Y. Z. C. CO., LTD
Changjiang economic development zone, Youxi
County, Fujian Province



Cartechnon GmbH
Neudorferstr. 71, 40474 Düsseldorf,
Germany



LOT 20200708

2020.07.08

18 MONTHS


Precauciones:

- Solamente para un único uso. La reutilización del dispositivo puede causar infección cruzada o protección insuficiente.
- No lo reutilice después de secar o desinfectar.
- Distinga correctamente la parte delantera y trasera antes de usar.
- Por favor, preste atención a la fecha de vencimiento del producto antes de su uso.
- Deseche adecuadamente las mascarillas usadas de acuerdo con la política local de eliminación de desechos médicos.
- El dispositivo no debe usarse durante más de 24 horas.
- Manténgalo alejado del fuego.
- No usar si es alérgico a telas no tejidas.

Mascarilla médica quirúrgica IIR desechable

INSTRUCCIONES DE USO

- Lavarse las manos con agua y jabón o frotarlas con una solución hidroalcohólica antes de manipular la mascarilla.
- Identificar la parte superior de la mascarilla.
- Colocar la mascarilla en la cara y ajustar la pinza nasal en la nariz.
- Sostener la mascarilla desde el exterior y pasar el arnés de cabeza o anudarlo detrás de la misma, a ambos lados de las orejas, sin cruzarlos.
- Bajar la parte inferior de la mascarilla a la barbilla y verificar que la mascarilla cubre la barbilla.
- Pellizcar la pinza nasal con ambas manos para ajustarla a la nariz y verificar que está colocada correctamente.
- Una vez ajustada, no tocar la mascarilla con las manos.

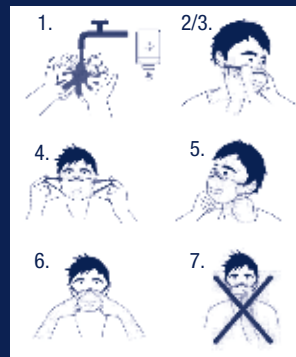

DISPOSABLE SURGICAL MASK IIR

Size : 17.5*9.5cm **BFE≥98%** **Pa/cm2<60**

Type IIR according to EN 14683:2019, YY/T0969-2013

Material Composition: 3Ply, Inner layer: PP non-woven (28%)
Middle layer: meltblown non-woven (34%)
Outer layer: PP non-woven (38%)

Medical Device: Fujian Pharmaceutical Supervision Machinery
Production License: Production No. 20200574 (provisional)

MASCARILLA QUIRURGICA IIR DESECHABLE



50 pcs/box

USO PREVISTO

Las máscaras faciales *médicas* deben usarse para proteger principalmente contra la propagación o transmisión de gérmenes infecciosos y agentes patógenos. El objetivo principal es proteger al paciente, y una de las características diferenciadoras de la mascarilla IIR es la protección adicional del usuario, que en ciertas situaciones se ve expuesto a salpicaduras de líquidos y microgotas potencialmente contaminantes y partículas viables.

- Protección de fluidos a pacientes y usuarios
- Suave y fácil de respirar
- No fabricado con látex de caucho natural

10 uds



MASCARILLA DESECHABLE QUIRÚRGICA IIR

DISPOSABLE SURGICAL MASK

Tamaño : 17.5*9.5cm **BFE≥98%** **Pa/cm2<60**

Instrucciones de uso

1. Lavarse las manos con agua y jabón o frotarlas con una solución hidroalcohólica antes de manipular la mascarilla.
2. Identificar la parte superior de la mascarilla.
3. Colocar la mascarilla en la cara y ajustar la pinza nasal en la nariz.
4. Sostener la mascarilla desde el exterior y pasar el arnés de cabeza o anudarlo detrás de la misma, a ambos lados de las orejas, sin cruzarlos.
5. Bajar la parte inferior de la mascarilla a la barbilla y verificar que la mascarilla cubre la barbilla.
6. Pellizcar la pinza nasal con ambas manos para ajustarla a la nariz y verificar que está colocada correctamente.
7. Una vez ajustada, no tocar la mascarilla con las manos.



Precauciones:

- a. Solamente para un único uso. La reutilización del dispositivo puede causar infección cruzada o protección insuficiente.
- b. No lo reutilice después de secar o desinfectar.
- c. Distinga correctamente la parte delantera y trasera antes de usar.
- d. Por favor, preste atención a la fecha de vencimiento del producto antes de su uso.
- e. Deseche adecuadamente las mascarillas usadas de acuerdo con la política local de eliminación de desechos médicos.
- f. El dispositivo no debe usarse durante más de 24 horas.
- g. Manténgalo alejado del fuego.
- h. No usar si es alérgico a telas no tejidas.

Composición:

3 Capas, Capa interna: PP non-woven (28%)
Capa intermedia: meltblown non-woven (34%)
Capa exterior: PP non-woven (38%)

Dispositivo médico

Fujian Pharmaceutical Supervision Machinery

Licencia de producción:

Production No. 20200574 (provisional)

Tipo IIR según EN 14683:2019, YY/T0969-2013



EC REP

LOT

Fecha de producción

Plazo de validez

F. Y. Z. C. CO., LTD
Chengxiyuan, economic development zone, Youxi
County, Fujian Province

生产厂商: 福建省尤溪县正泉布业有限公司
生产地址: 福建尤溪经济开发区城西园

Caretechion GmbH
Niederrheinstr 71, 40474 Duesseldorf,
Germany